

FIGURE 7 Residual *tert*-butanol levels in annealed versus non-annealed CAVERJECT Sterile Powder.

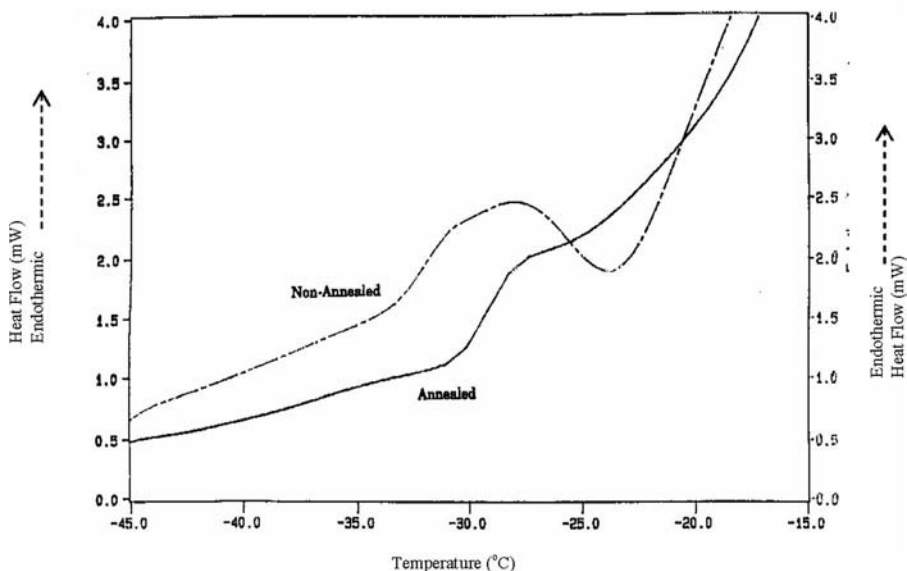


FIGURE 8 Differential scanning calorimetry thermograms for annealed versus non-annealed bulk solution used in CAVERJECT Sterile Powder.